


Omega Optical Inc
Instrument Serial Number EL 05084038



XBSSL, BESSELL "U", #69519 GWJ

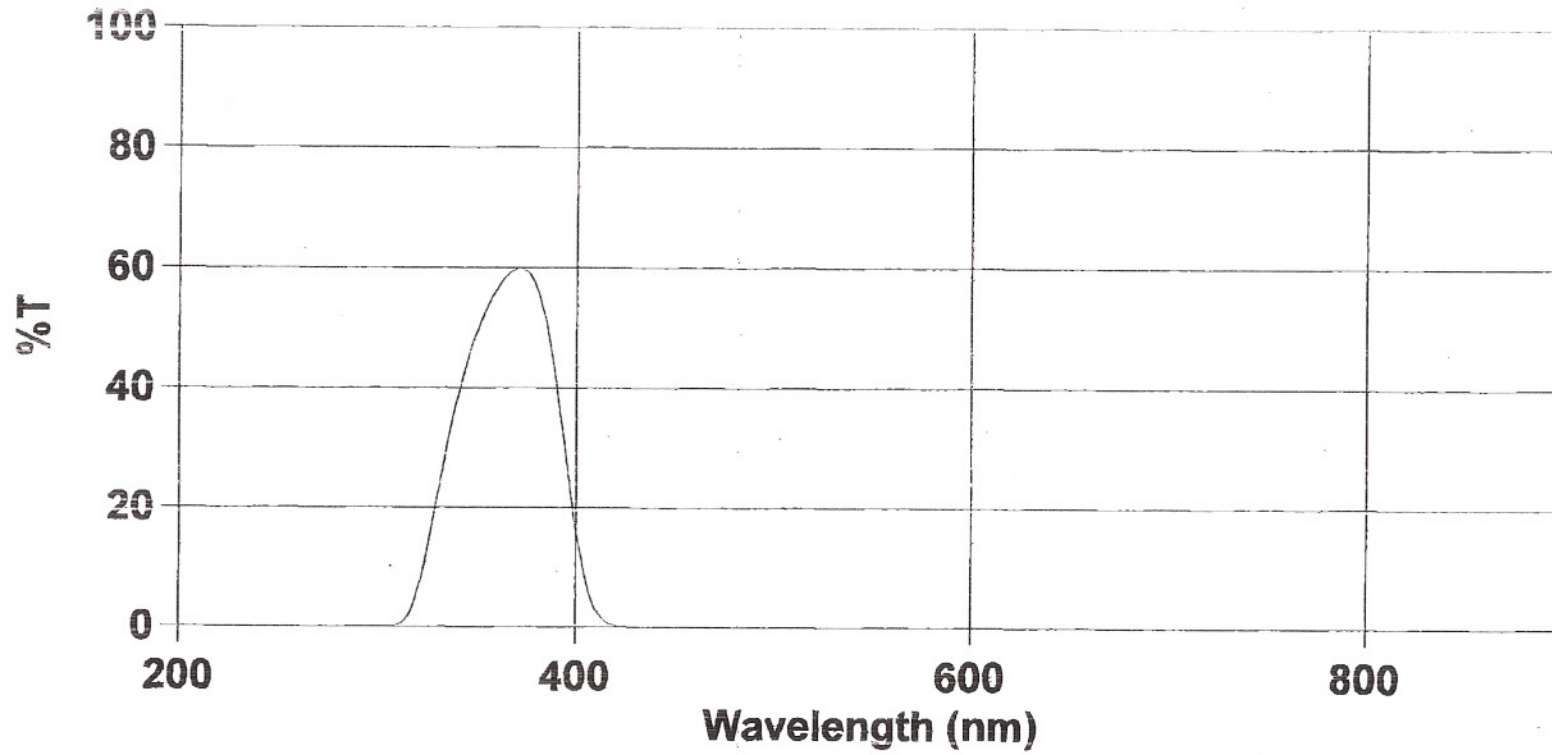

Omega Optical, Inc.
 21 Omega Drive
 Brattleboro, VT 05301 USA
 Toll Free: (866) 488-1064
 Phone: (802) 254-2690
 Fax: (802) 254-3937

Packing List

Date: 11/26/2007

Account: CU/000300
 Name: Tel Aviv University
 Order: SO/076004
 Cust PO: 06 6010762

Ship To:

Tel-Aviv University
 C/O UTI
 60 Brunswick Avenue
 Edison, NH 08817
 United States
 Attn: Mr. Rafi Dabush
 Phone: 972-3-6408627
 PO# 06 6010762 SO/076004

Sold To:

Tel Aviv University
 P.O. Box 39040, Import Department
 Tel Aviv, 61390
 Israel
 Attn: Accounts Payable


Order Terms: Net Due 45 Days
 Ship Via: FedEx Standard Overnight
 Frt Terms: Prepaid
 Ship Acct: 105051220

CERTIFICATE OF QUALITY AND QUANTITY		CUSTOMER REFERENCE		ORDER NUMBER/LINE	PART NUMBER/DESCRIPTION
QTY	BATCH #/DATE CODE	QTY REC.	INITIALS		
				SO/076004/001	Omega PN: XBSSL/U/50S Descr: Standard Photometry/Imaging Cust PN:
				Ship On 10/03/2007	Due 1
					Shipped <u>1</u>

The materials delivered under the above captioned order have been inspected and found to be in compliance with the specifications of the order and meet requisite standards of workmanship.

Date & Time Printed: 11/26/2007 12:27 pm

Total





Filter – Instructions

Handling

- THIS FILTER SHOULD BE HANDLED AT THE EDGES ONLY.
- Exposed coatings can be softer than glass and can easily be scratched if handled improperly.

Cleaning

- This filter was cleaned and inspected prior to shipment. If additional cleaning is necessary, it should be done carefully.
- Any dust or foreign material can be removed using dry air under pressure.
- A very light, wiping motion using a soft, lint-free cloth should remove any remaining particles.
- A final cleaning with a few drops of pure, anhydrous alcohol or acetone on a fresh lab towel will result in a clean, undamaged component.
- Hard, refractory oxide coatings will withstand many cleanings.

Filter Orientation

- Filters should be installed with the arrow pointing in the direction of the light path (or pointing away from the light source).
- Dichroic filters should be oriented with the reflective coating toward the light source. (They are marked on the side opposite the coating, which should be positioned away from the light source).